



1/17

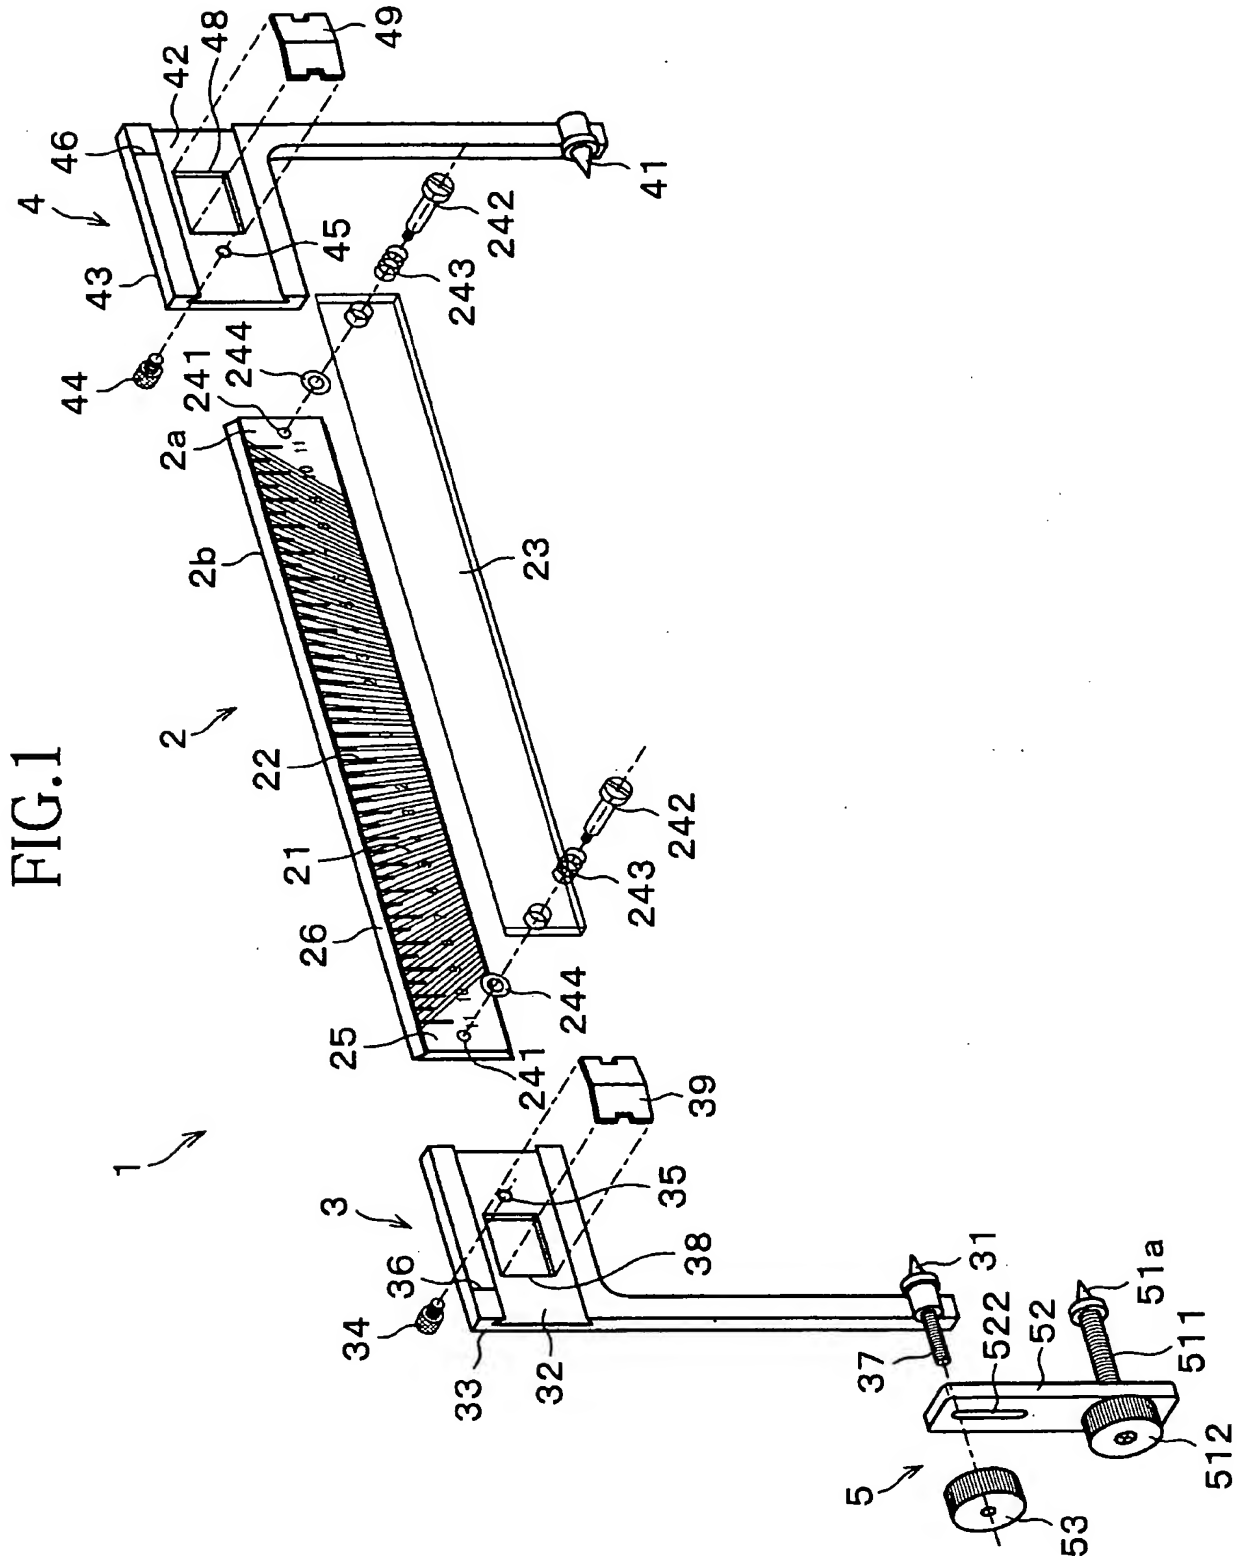

Appl. No.: Unknown Atty Docket: TSU-005

FIG. 2

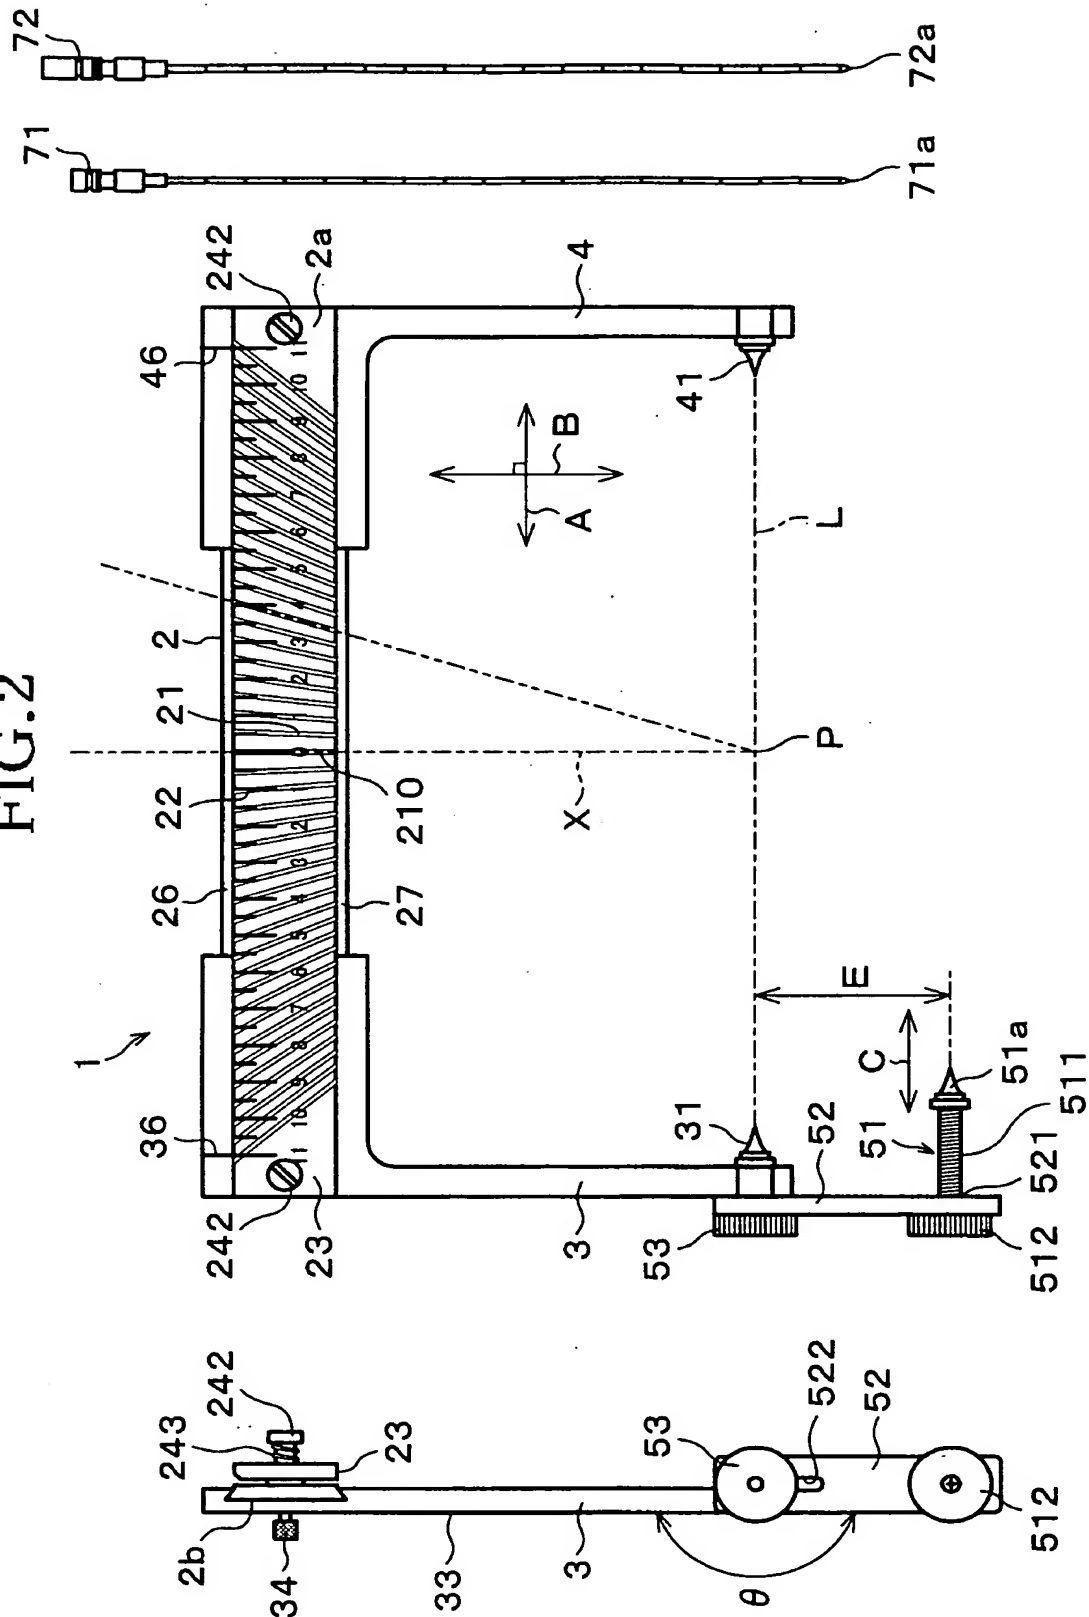


Hiroyuki TAI

Appl. No.: Unknown

Atty Docket: TSU-005

3/17

FIG.3

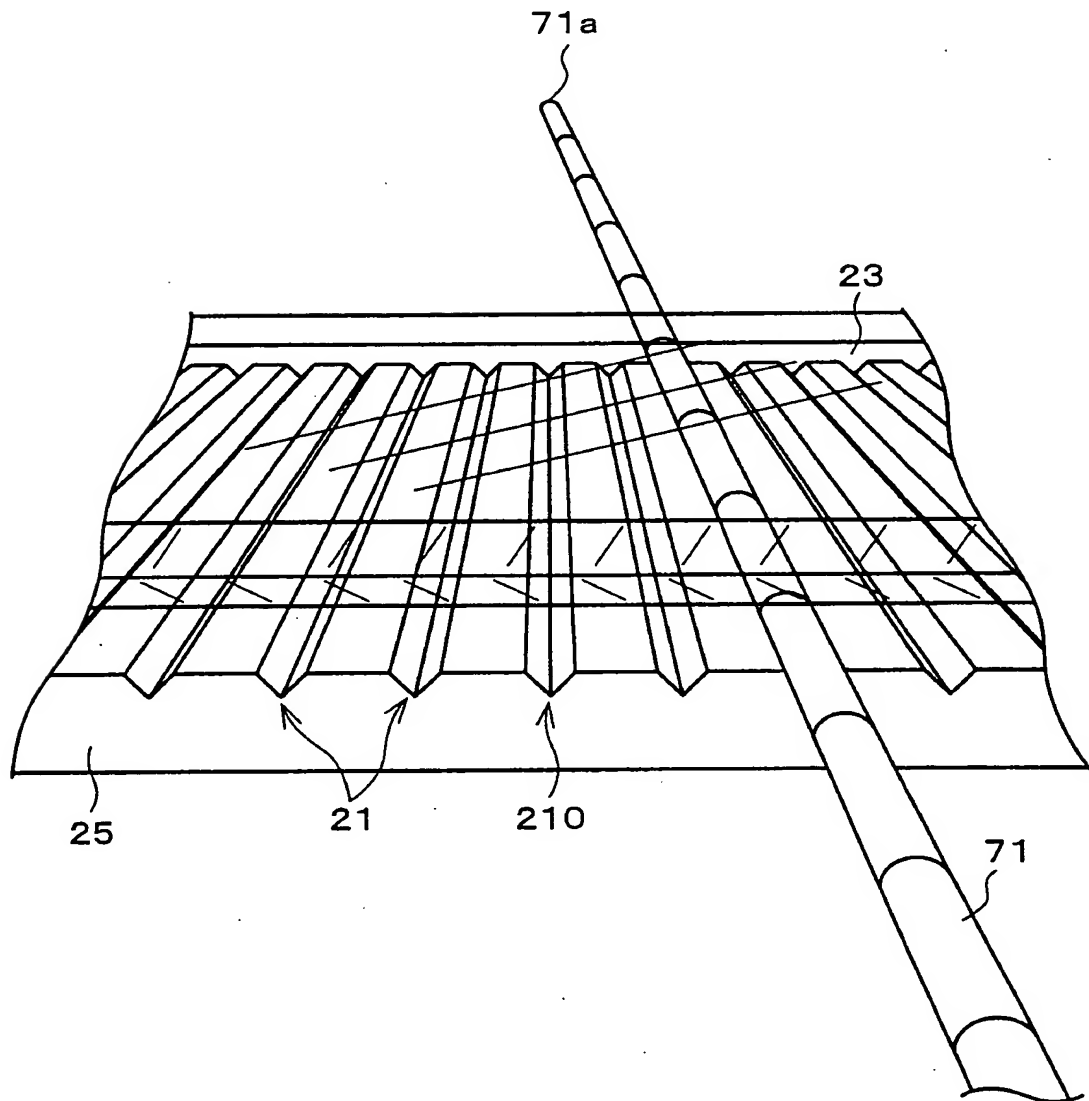

SIMPLIFIED STEREOTACTIC BRAIN SURGERY DEVICE, AND
BAND USED FOR DETERMINING POSITION AT WHICH SUCH
DEVICE IS MOUNTED ON PATIENT HEAD

Hiroyuki TAI


Appl. No.: Unknown


Atty Docket: TSU-005

10/526805

4/17

FIG. 4

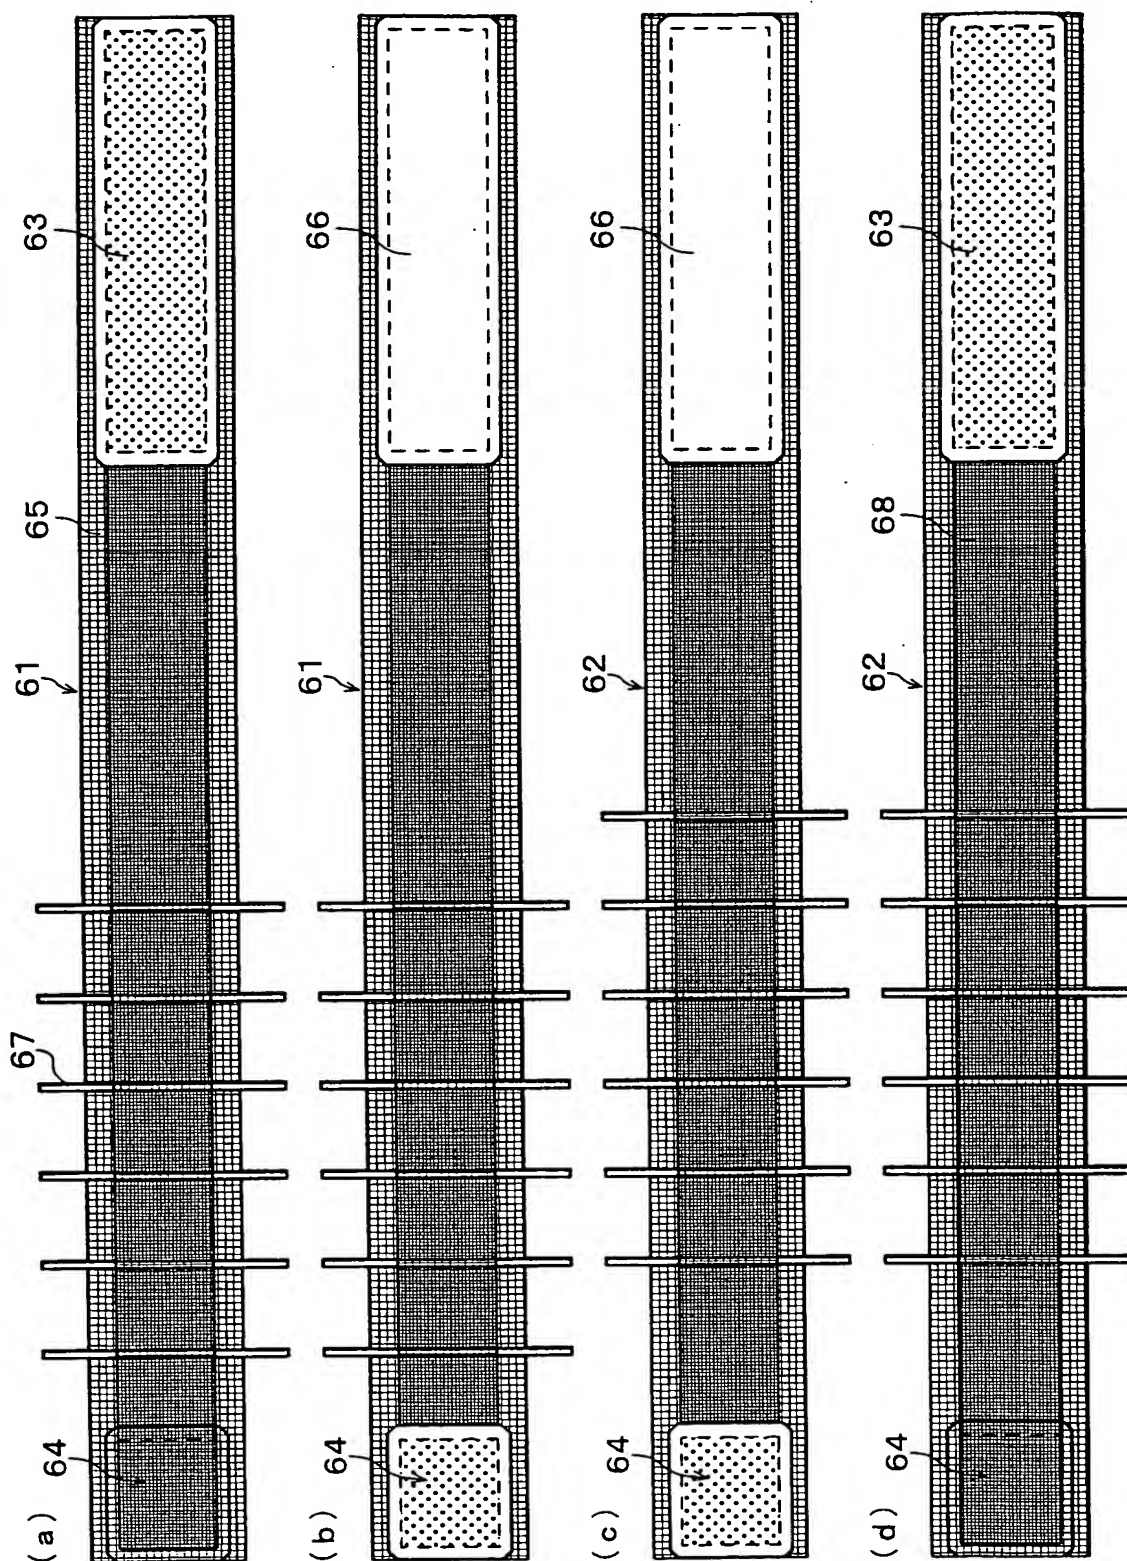

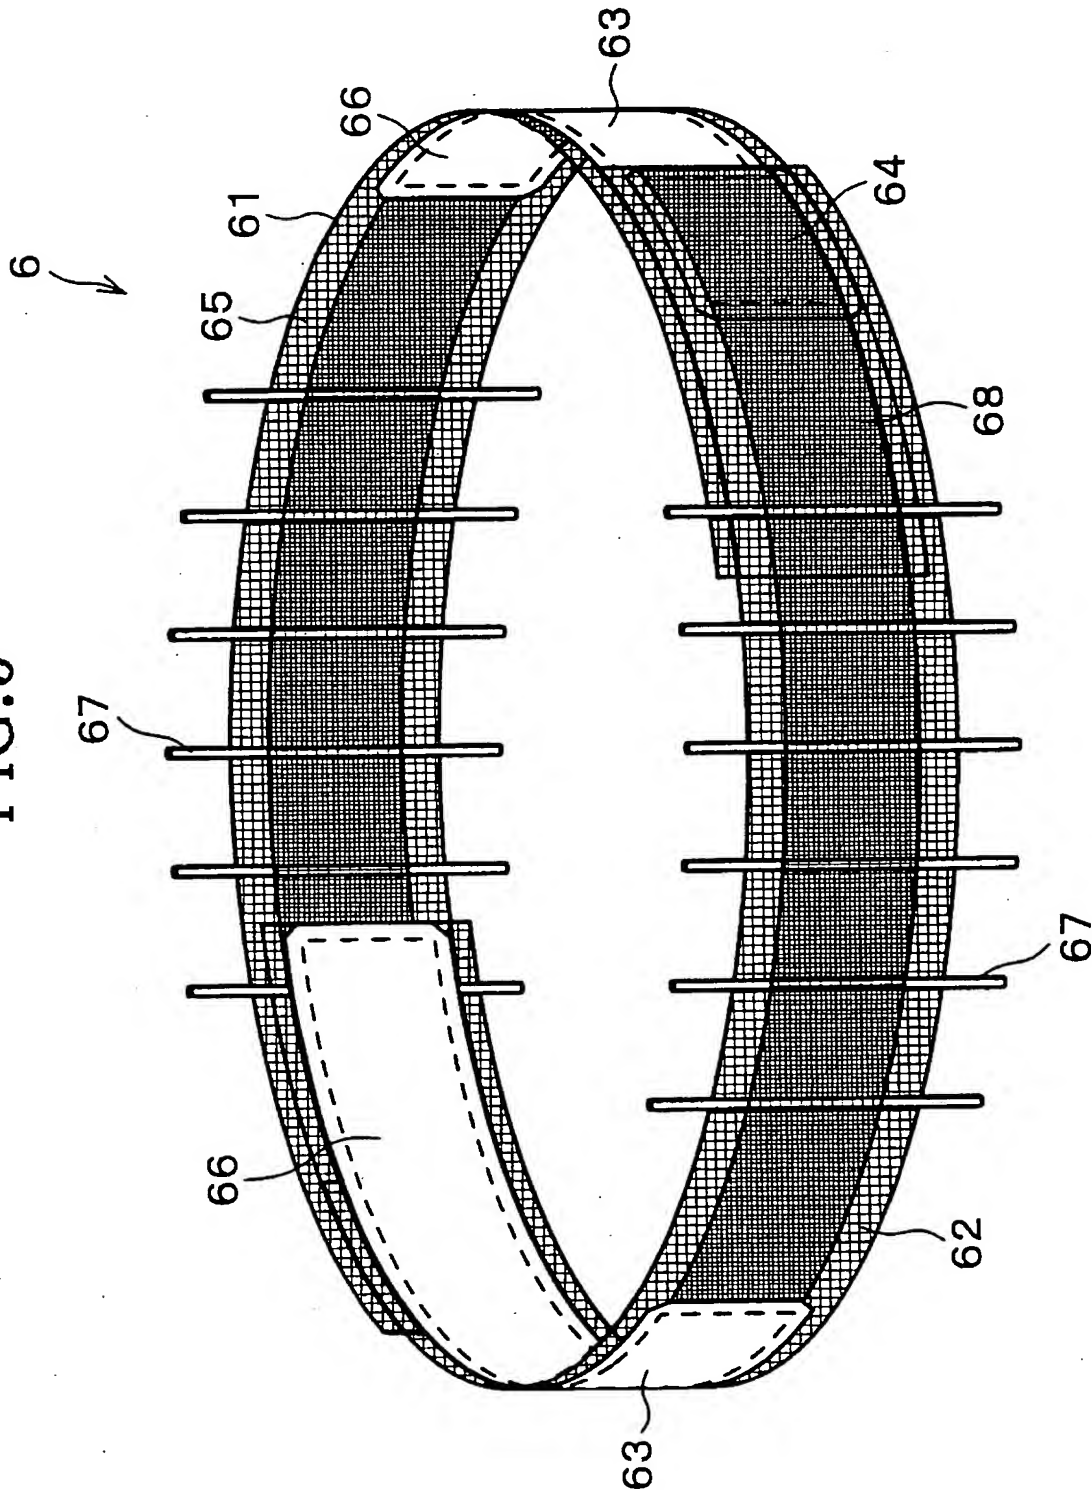

Hiroyuki TAI


Appl. No.: Unknown

Atty Docket: TSU-005


6/17

FIG.6


(a)

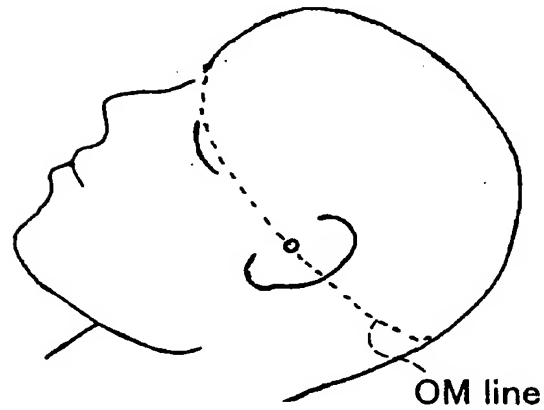

(b)

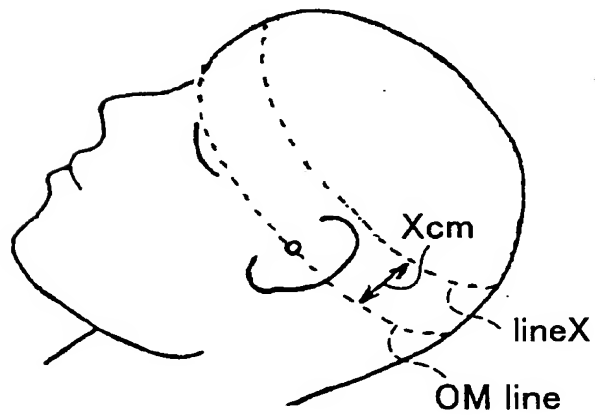


(c)

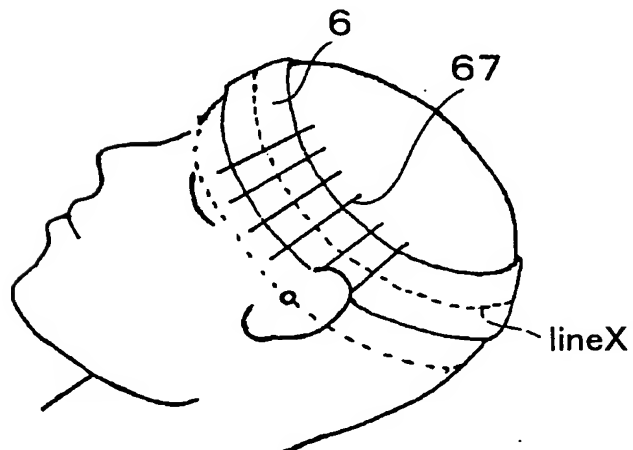


7/17

FIG. 7

(a)

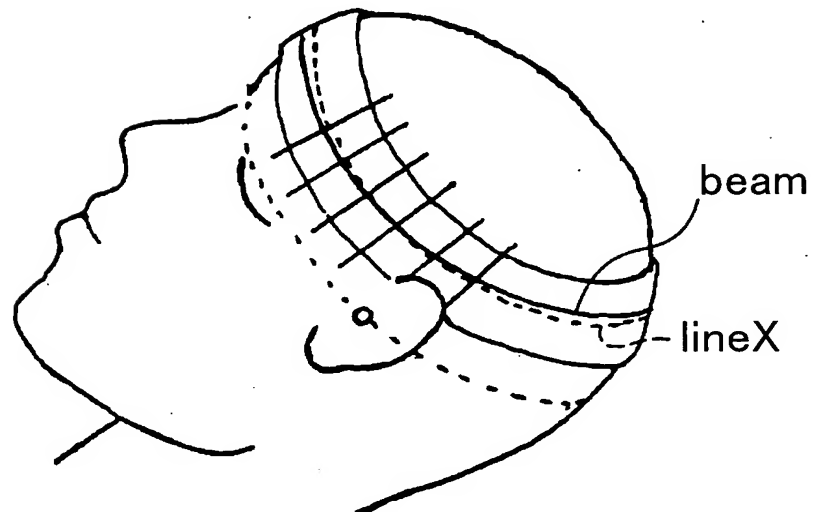


(b)

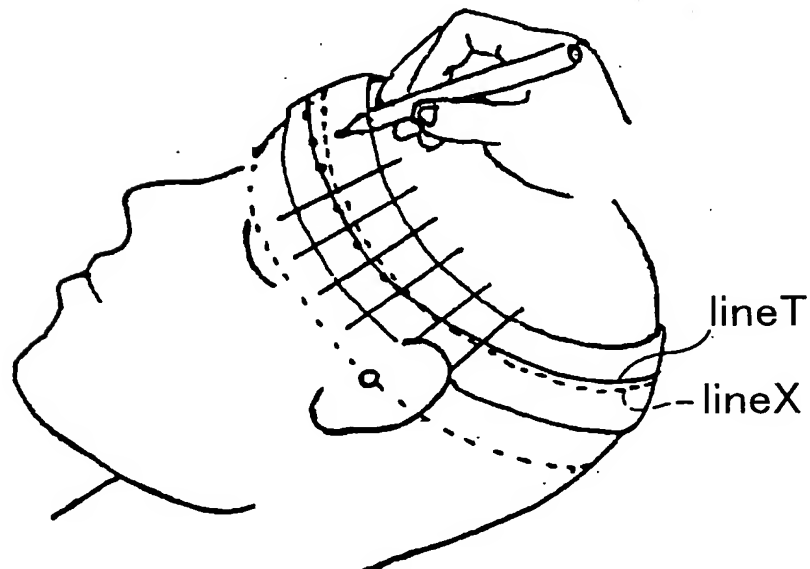


8/17

FIG.8

(a)

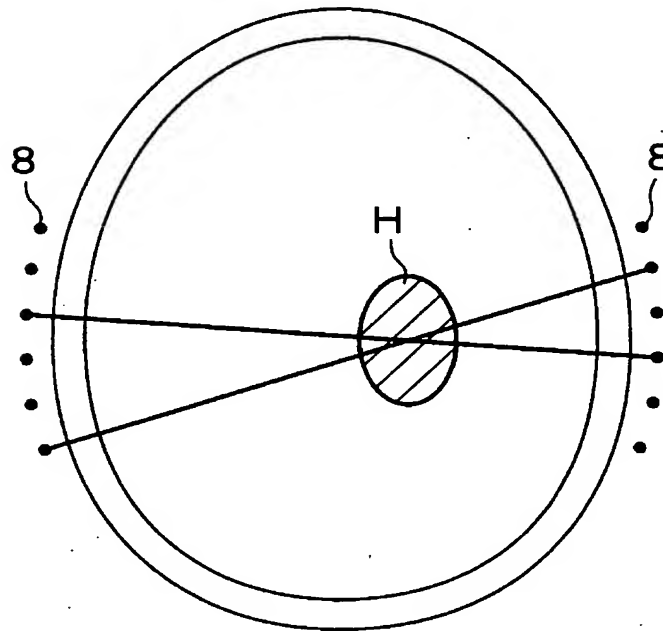

(b)

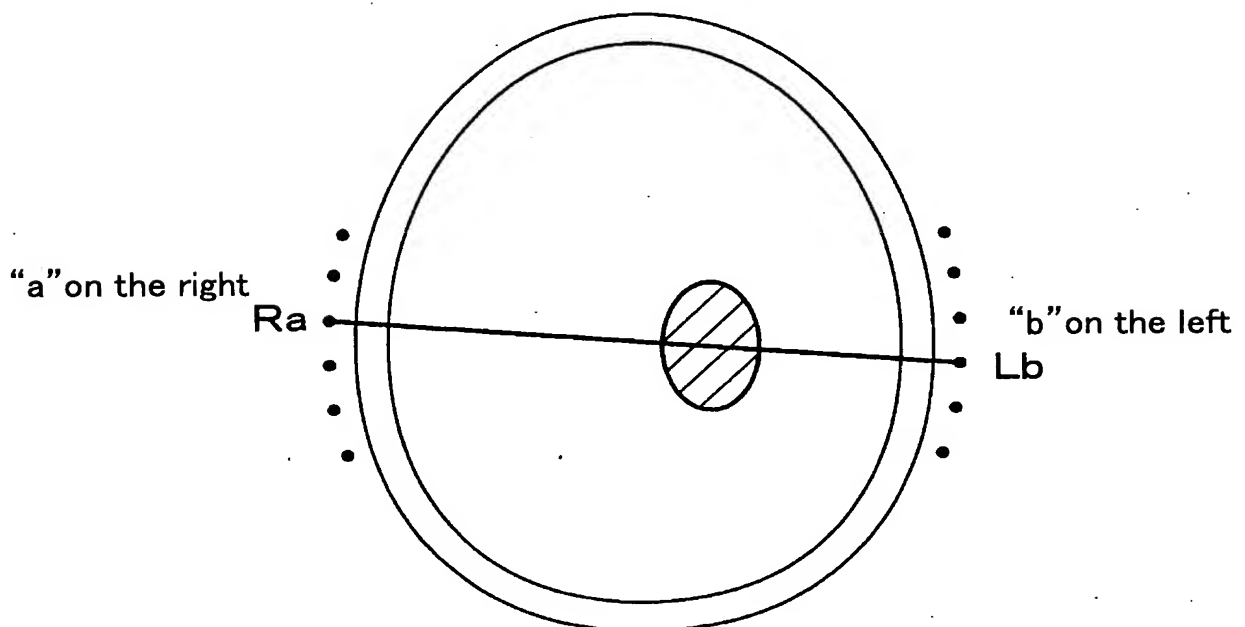

Hiroyuki TAI


Appl. No.: Unknown

Atty Docket: TSU-005


9/17

FIG.9

(a)

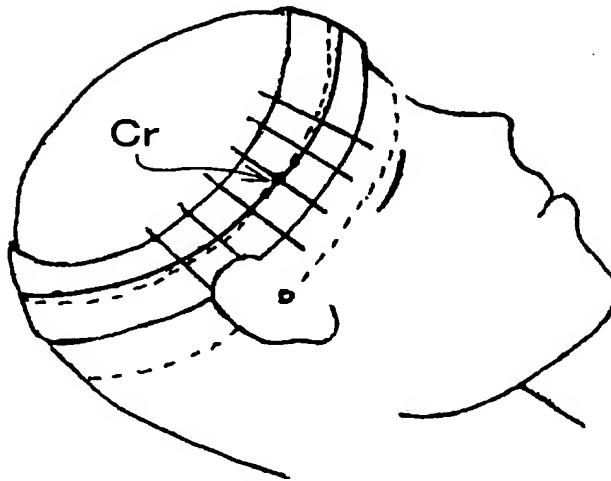

(b)

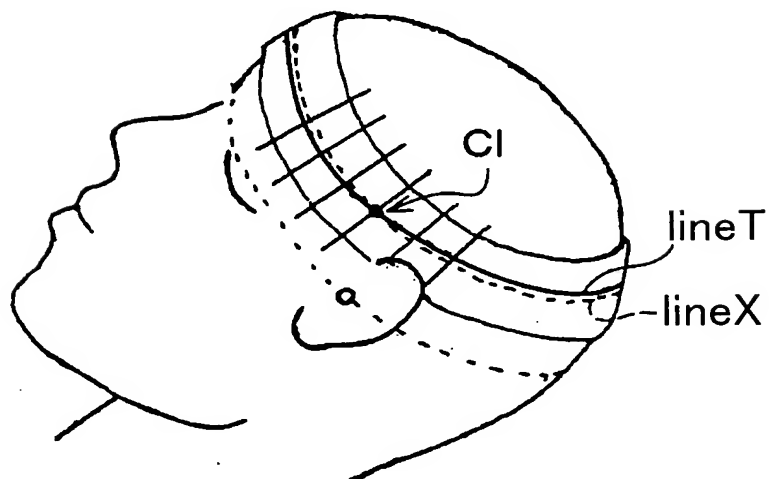

Hiroynki TAI


Appl. No.: Unknown

Atty Docket: TSU-005

10/17


FIG.10

(a)

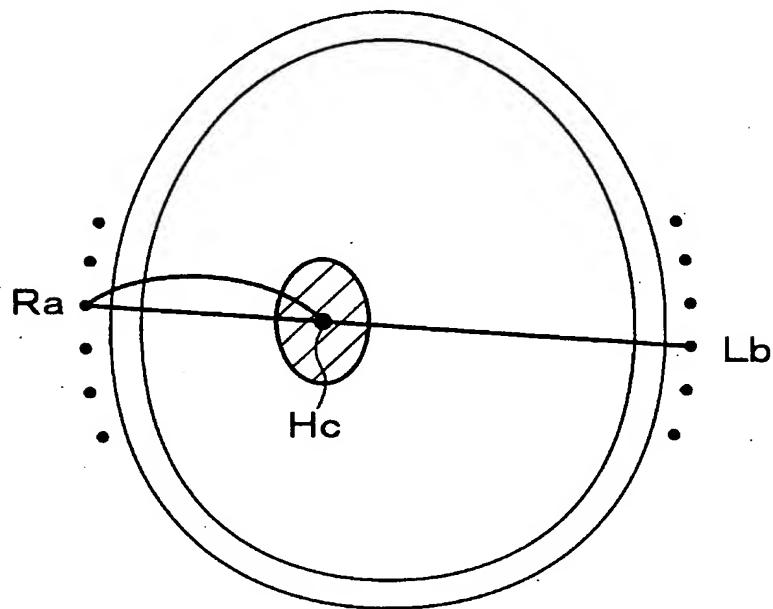

case of right hematoma

(b)

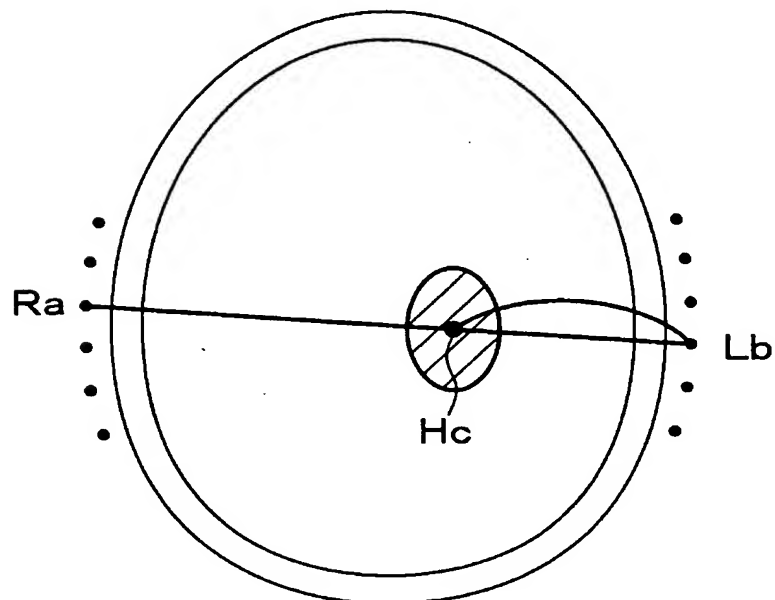

case of left hematoma

Hiroyuki TAI


Appl. No.: Unknown

Atty Docket: TSU-005


11/17

FIG.11

(a)

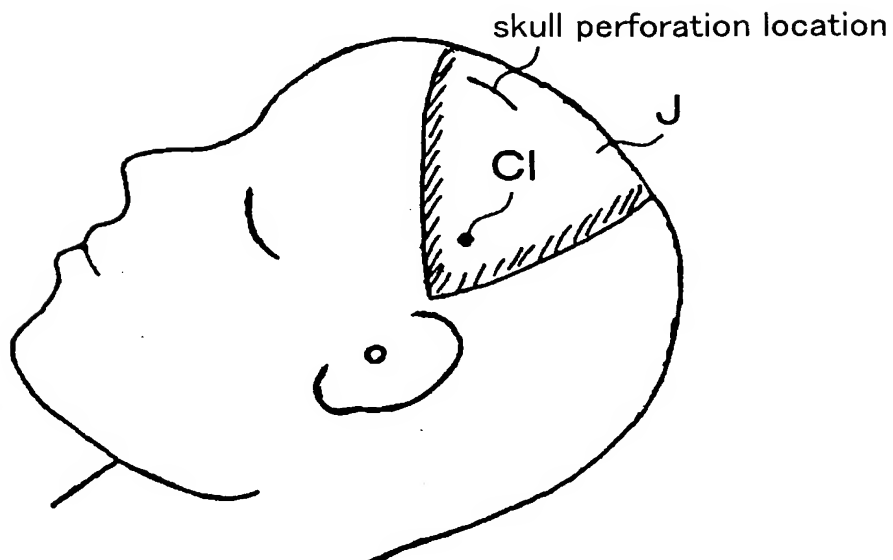


(b)

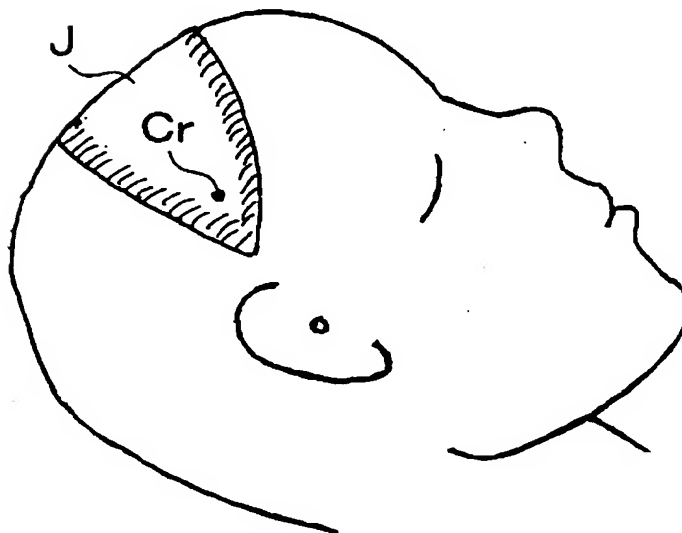

12/17

FIG.12

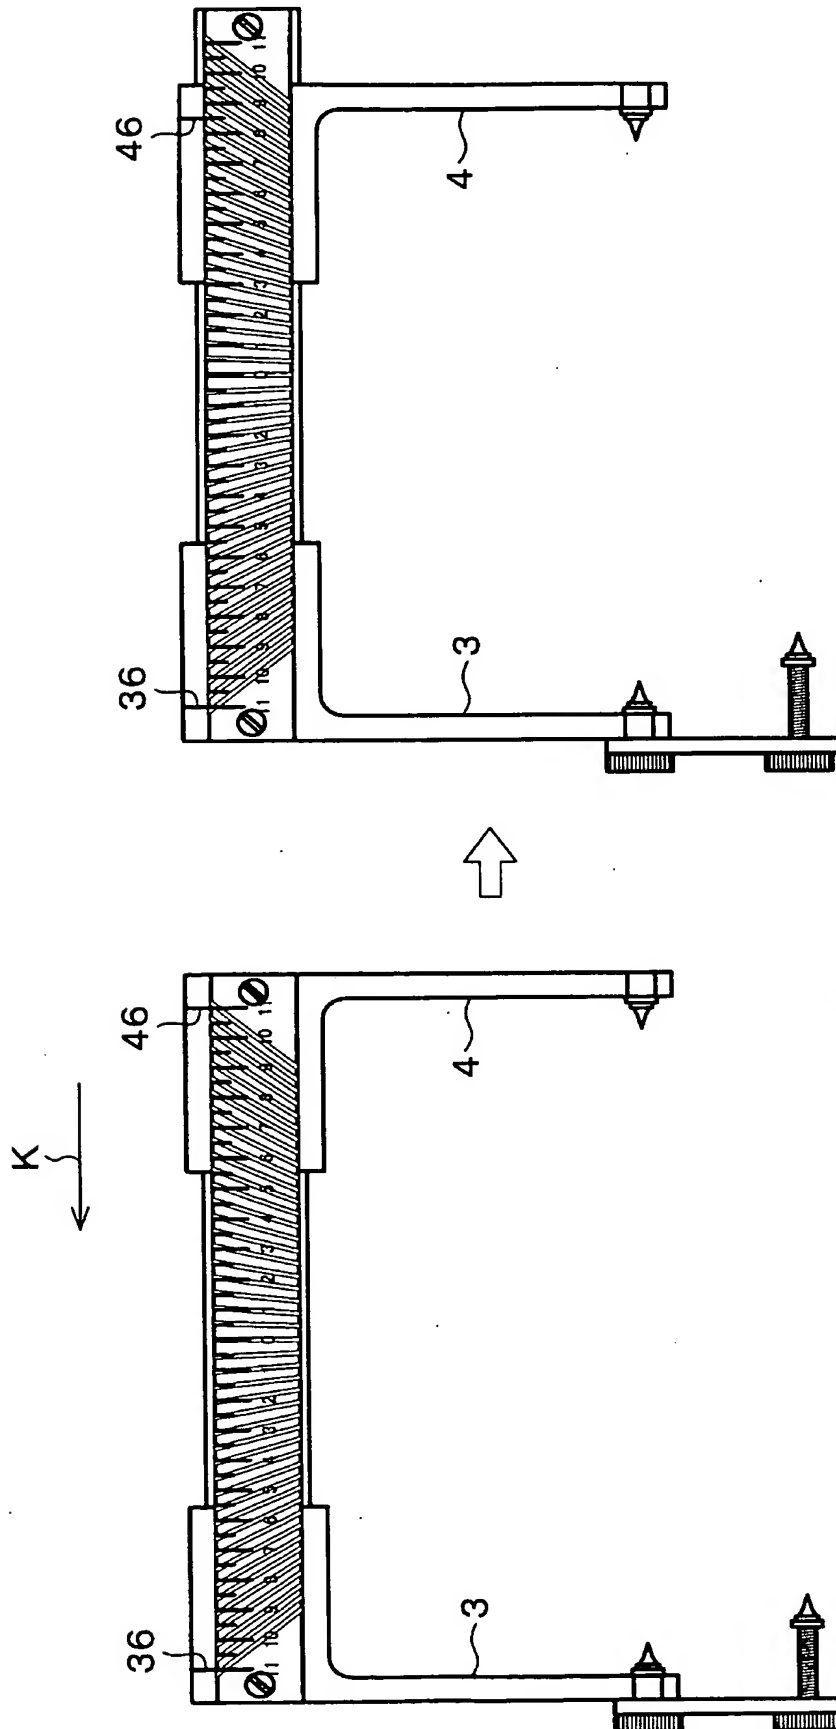


Hiroyuki TAI

Appl. No.: Unknown

Atty Docket: TSU-005

13/17

FIG.13

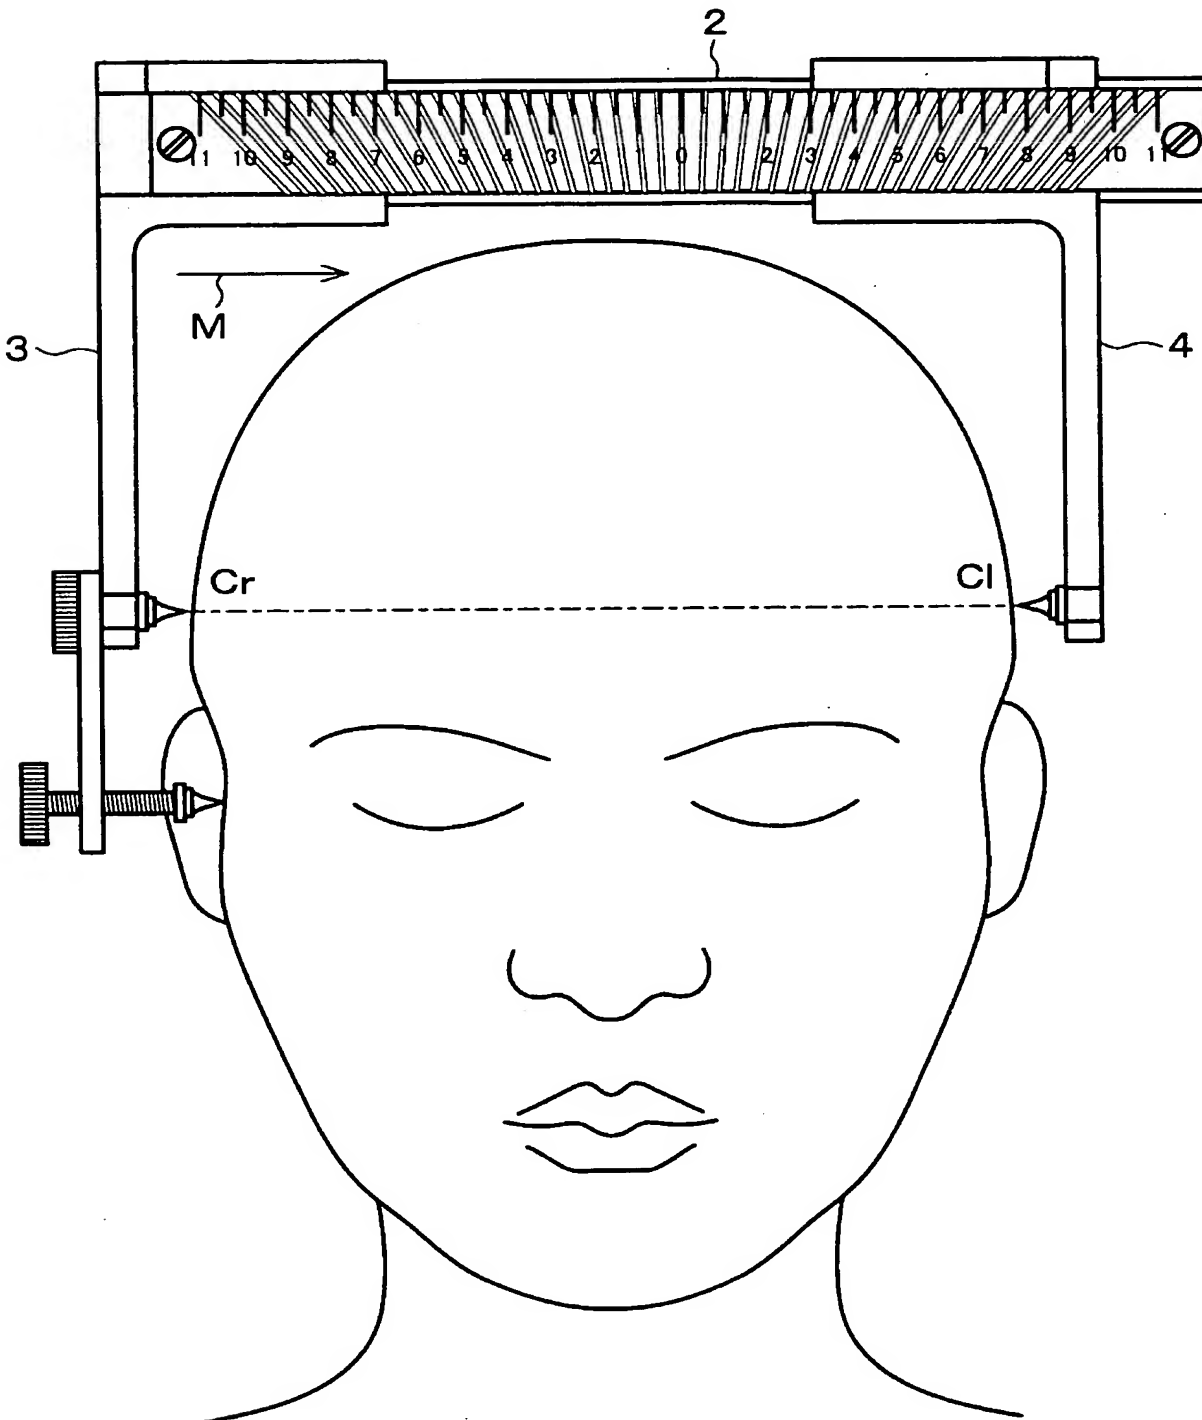


SIMPLIFIED STEREOTACTIC BRAIN SURGERY DEVICE, AND
BAND USED FOR DETERMINING POSITION AT WHICH SUCH
DEVICE IS MOUNTED ON PATIENT HEAD

Hiroyuki TAI

Appl. No.: Unknown Atty Docket: TSU-005


14/17

FIG.14

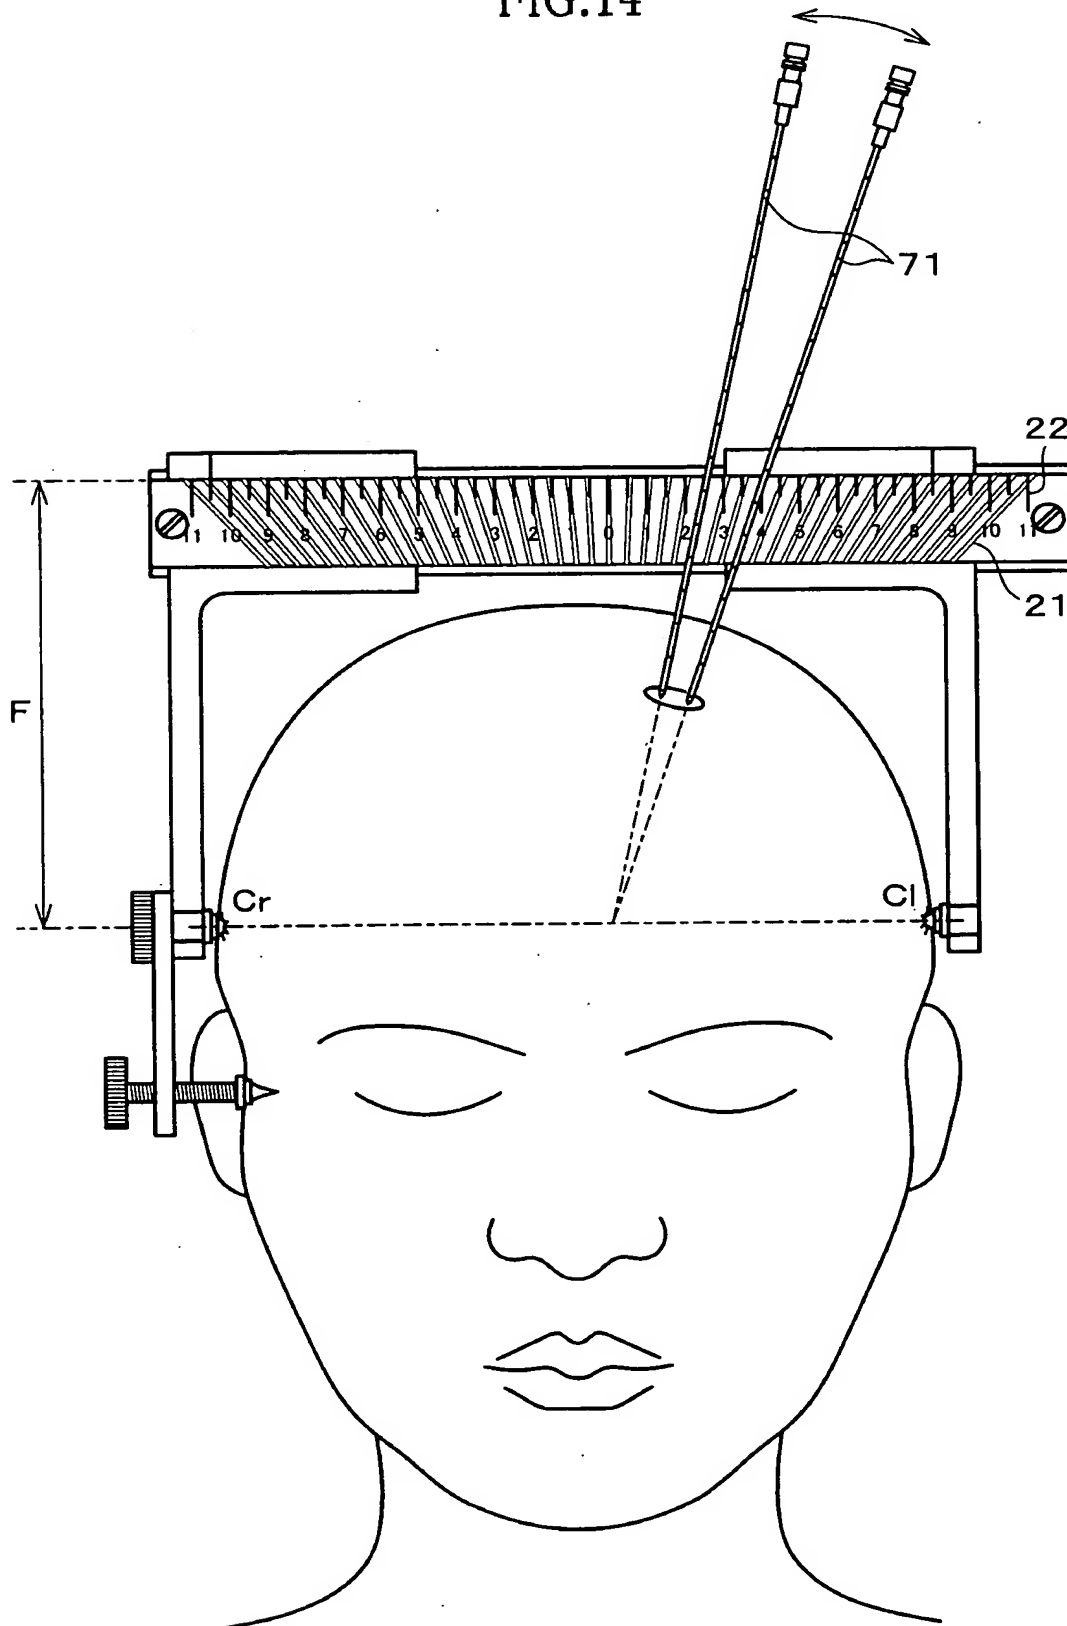

15/17

FIG.15

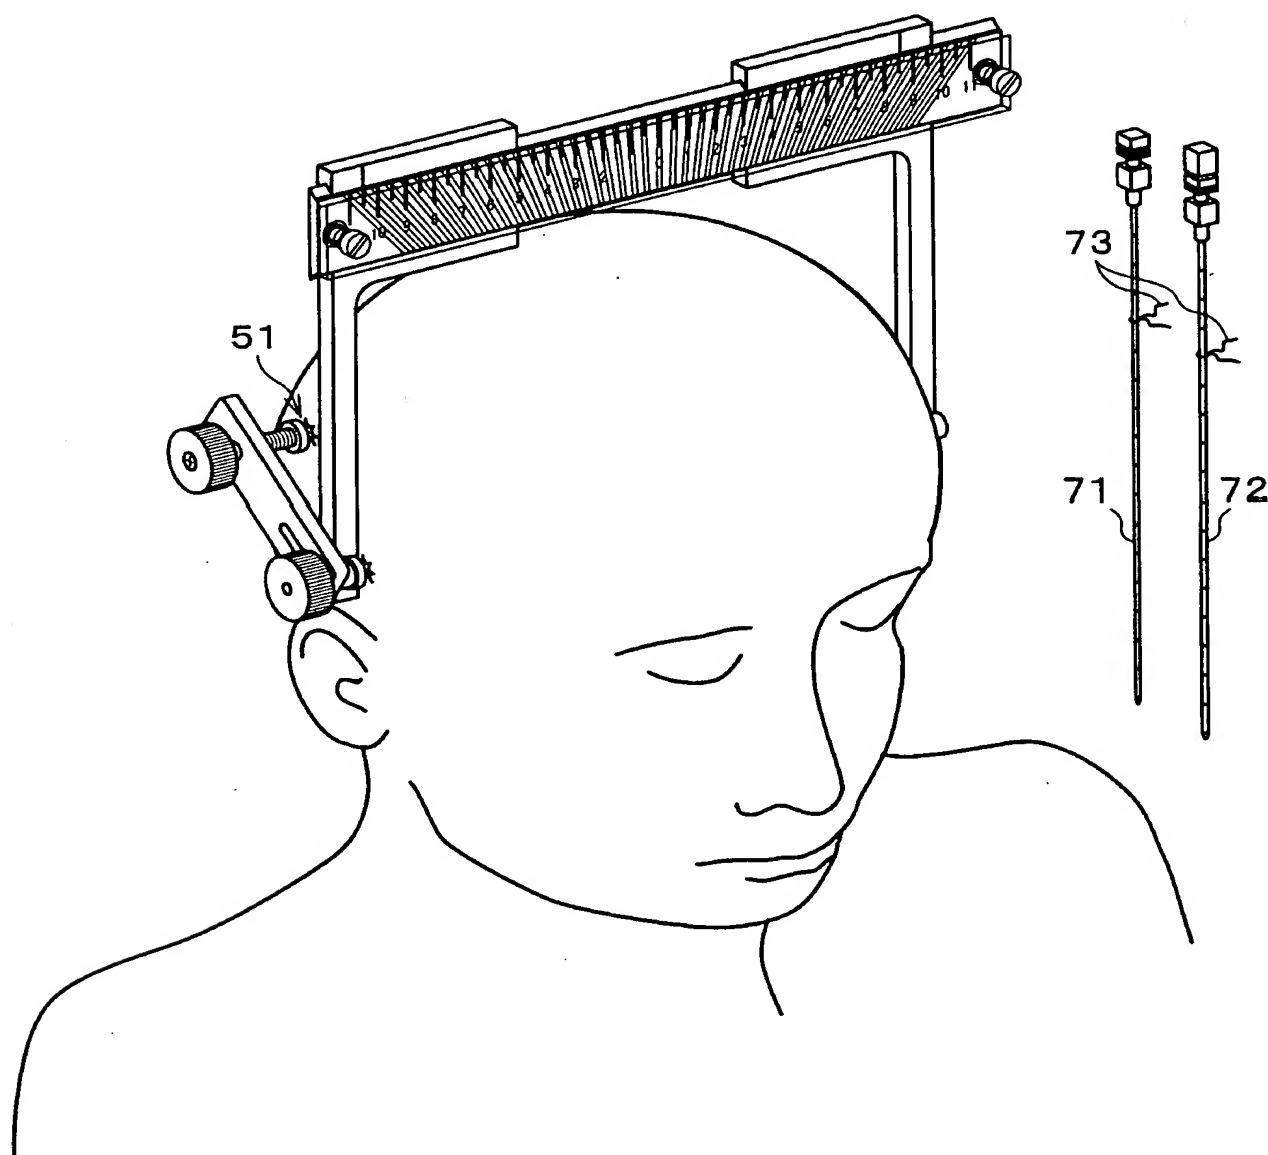


Hiroyuki TAI

Appl. No.: Unknown

Atty Docket: TSU-005

16/17

FIG. 16

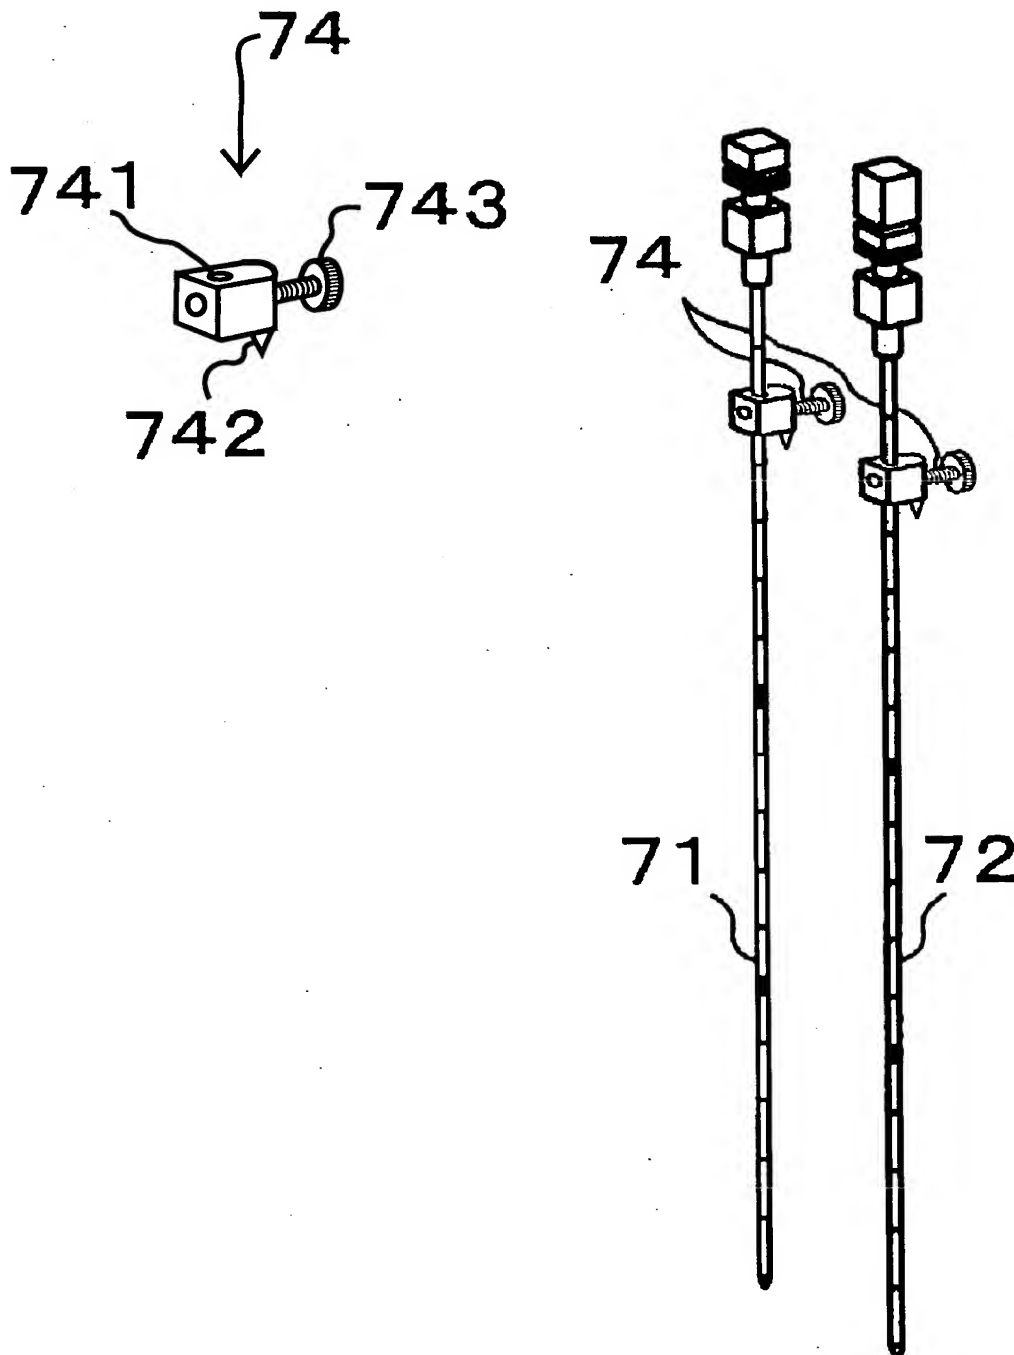

Appl. No.: Unknown Atty Docket: TSU-005

FIG. 17

